

TRACE GAS MONITOR

GA-370



Continuous and ultrahigh-sensitivity
measurement of trace impurities
(CO, CO₂ and CH₄) in high-purity gas

For monitoring quality control of manufactured high-purity gases at air separation and semiconductor plants

GA-370 provides constant, ultrahigh-sensitivity and high-precision monitoring of trace impurities (CO, CO₂ and CH₄) for quality control at gas manufacturing facilities.

Ultra-high Sensitive Measurements

- ▶ A cross-flow modulation dual-beam non-dispersive infrared (NDIR) analyzer provides continuous and stable zero drift-free measurements.
- ▶ Minimum detection limit (MDL) of 10 ppb which can support applications where high accuracy measurements are required.

Measurement of trace impurities in a balance gas

- ▶ Representative gases such as N₂, O₂, He, Ar, H₂ and Air are supported.


* For other balance gases, please contact HORIBA.

Easy maintenance-free operation

- ▶ Operator friendly screen menus simplify analyzer operation, calibration and measurements.
- ▶ No optical alignment ever required.
- ▶ A touch color LCD display allows operators to view graphs of accumulated data.



Typical Application

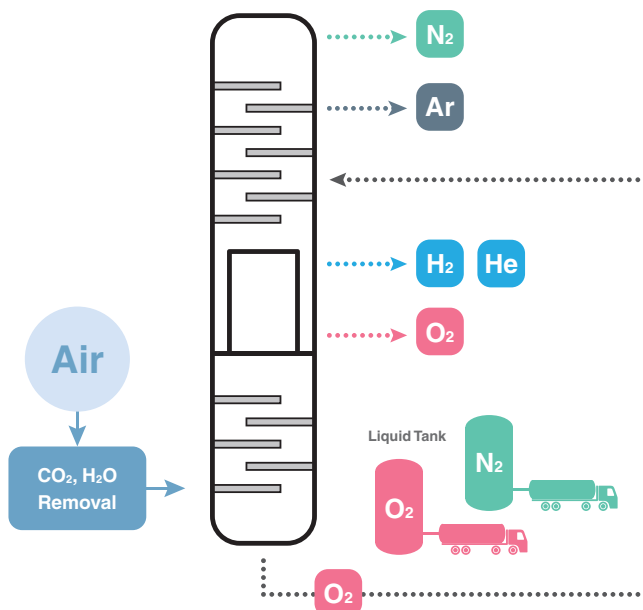

Industrial gases such as oxygen and nitrogen are manufactured by an air separation plant.



First, air that has had moisture (H₂O) and carbon dioxide (CO₂) is removed and separated to manufacture nitrogen (N₂), argon (Ar) and Oxygen (O₂). The separation process is based upon differences in boiling points of each of the constituent gases. Similarly, air separation plants manufacture other rare or inert gases such as Hydrogen (H₂) and Helium (He).

The HORIBA GA-370 Trace Gas Analyzer is a useful tool for measuring impurities that may be in the separated gas for quality control purposes.

Cross-flow modulation dual-beam non-dispersive infrared analyzer

The GA-370 Trace Gas Analyzer uses an infrared beam that passes through the cell to the detector. During measurement, a solenoid valve alternately directs the sample gas and the reference gas to the cells within the analyzer.

The presence of CO, CO₂ and/or CH₄ in the sample gas generates a difference in the intensity of light reaching the detector when the cell is filled with sample gas as compared to when the cell is filled with reference gas. The differences in absorption by the detector of the light from the two gases results in deflection of the detector's membrane to oscillate. This measurement technique eliminates any need for an optical chopper or optical adjustments as it eliminates zero drift and enhances sensitivity.

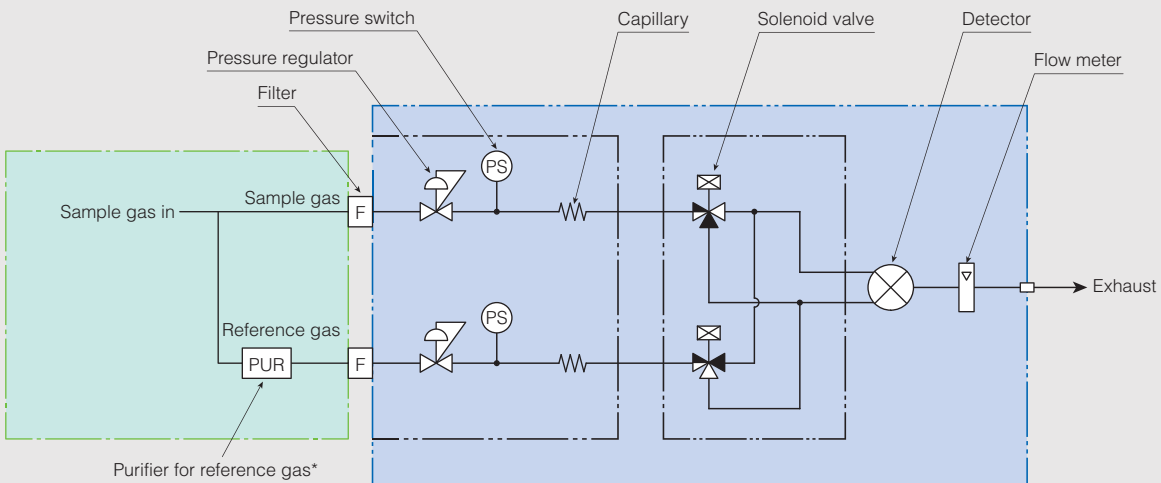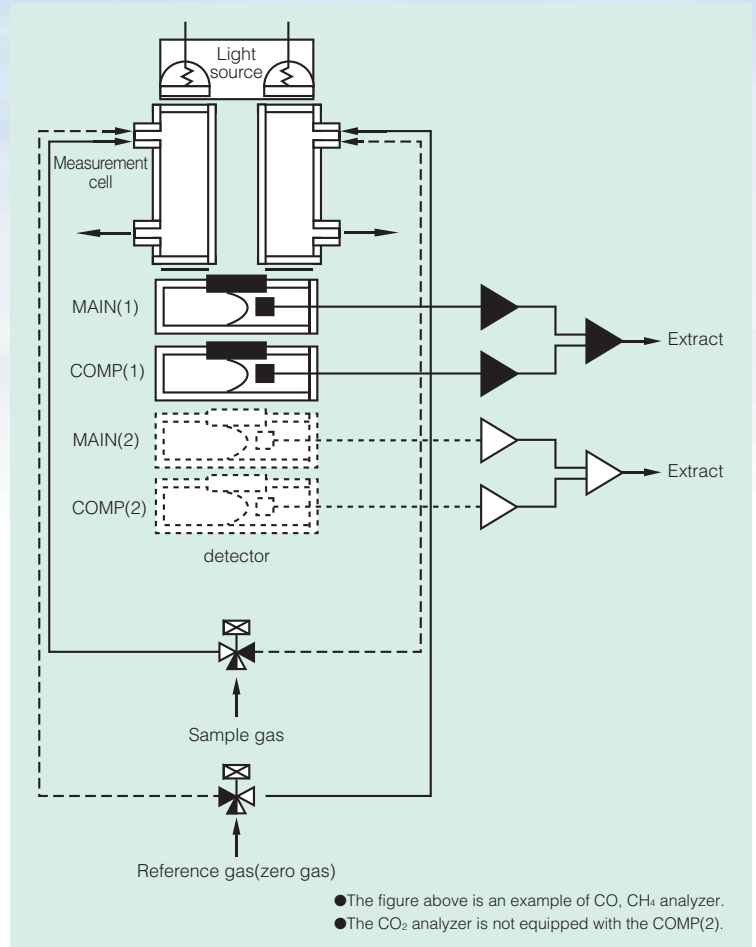

Customers are requested to provide components in the bulk gas.
 * When it is impossible to secure the purity of reference gas in Table 1, a reference gas purifier is required.

Table 1: List of reference gases (balance gas is to be same as the sample gas)

Measured Gas	Allowable concentrations of impurities (ppb)			
	H ₂ O	CO	CO ₂	CH ₄
CO analyzer	5000	10	1000	1000
CO ₂ analyzer	5000	1000	10	1000
CH ₄ analyzer	5000	1000	1000	10

GA-370 Specifications

Model	GA-370
Gases measured	CO, CO ₂ , and CH ₄
Bulk gases	N ₂ , O ₂ , He, Ar, H ₂ , Air
Number of measurement components	1 component or 2 components (specify a measuring balance gas)
Measuring principle	Cross-flow modulation non-dispersive infrared (NDIR) absorption method
Measurement ranges	0 to 1/2/5/10 ppm
Lowest detection limit (2σ)	10 ppb
Repeatability	≤±2% of full scale
Indication error	≤±2% of full scale
Zero Drift	≤±0.02 ppm/day, ≤±0.03 ppm/week
Span Drift	≤±2% of full scale/day, ≤±3% of full scale/week
Response time (T ₉₀)	≤180 s

Gas flow rate *	Sample gas: approx. 3.5 L/min, reference gas: approx. 3.5 L/min, span gas: approx. 3.5 L/min Note: A delivery pressure of 50-100 kPa is recommended for both sample and reference gas.	
Analog output	Max. 2 channels isolated output (2 components) Select one from 0 to 1 V, 0 to 10 V, 0 to 16 mA, 4 to 20 mA, or 0 to 20 mA Current output: Allowable load resistance 750Ω or less	
Installation conditions	Ambient temperature	0 to 40°C
	Ambient relative humidity	≤85%
	Dust	Less than environmental standard
	Vibration	≤0.29 m/s ² , at ≤100 Hz
"External dimensions, weight"	430(W) × 221(H) × 555(D) mm (excluding protrusions), approx. 18 kg	
Power supply	100 to 240 V AC, ≤±10%(max. voltage: 250 V AC)	
Power consumption	Approx. 100 VA	

* Note 1) Customers are required to provide reference and span gases. The purity of the measured bulk gas must equal to or lower than 0.1% of the analyzer's minimum range. A 9 ppm span gas is recommended for most applications.

* Note 2) The GA-370 Trace Gas Analyzer is not intrinsically safe. When measurements are made in an explosive gas such as H₂, the customer is required to implement proper precautions by locating the analyzer within a purged enclosure to avoid explosive conditions.

Related Products



Portable Gas Analyzer PG-300 Series

Measurement of max. 5 different components by single portable, lightweight and robust unit. Used for emission monitoring, R&D(fuel cell), stack cross check.

NO_x SO₂ CO CO₂ O₂ CH₄



Air Pollution Monitor AP-370 Series

Monitoring of ambient air pollutants: harmful oxides and particulate. Used for ambient air, clean room, indoor air and trace gas monitoring.

O₃ SO₂ NO_x CO NH₃ H₂S THC NMHC CH₄
SPM PM_{2.5} PM₁₀



Multi-Component Gas Analyzer VA-5000 Series

Supports diverse needs from environmental problems to energy development support. Up to 4 components can be measured by one unit.

CO CO₂ N₂O CH₄ SO₂ NO NO_x O₂ NH₃



The HORIBA Group adopts IMS (Integrated Management System) which integrates Quality Management System ISO9001, Environmental Management System ISO14001, and Occupational Health and Safety Management System OHSAS18001. We have now integrated Business Continuity Management System ISO22301 in order to provide our products and services in a stable manner, even in emergencies.



Please read the operation manual before using this product to assure safe and proper handling of the product.

- The specifications, appearance or other aspects of products in this catalog are subject to change without notice.
- Please contact us with enquiries concerning further details on the products in this catalog.
- The color of the actual products may differ from the color pictured in this catalog due to printing limitations.
- It is strictly forbidden to copy the content of this catalog in part or in full.
- The screen displays shown on products in this catalog have been inserted into the photographs through compositing.
- All brand names, product names and service names in this catalog are trademarks or registered trademarks of their respective companies.

<http://www.horiba.com> e-mail: info@horiba.co.jp

HORIBA, Ltd. Japan

Head Office
2 Miyano Higashi, Kisshoin, Minami-ku, Kyoto, Japan
Phone: 81 (75) 313-8121 Fax: 81 (75) 321-5725

HORIBA (China) Trading Co., Ltd. China

Shanghai
Unit D, 1F, Building A, Synnex International Park, 1068 West Tianshan Road, Shanghai, 200335, China
Phone: 86 (21) 6289-6060 Fax: 86 (21) 6289-5553
Beijing
12F, Metropolis Tower, No.2, Haidian Dong 3 Street, Beijing, 100080, China
Phone: 86 (10) 8567-9966 Fax: 86 (10) 8567-9066

HORIBA Korea Ltd. Korea

10, Dogok-Ro, 6-Gil, Gangnam-Gu, Seoul-Si, 06259, Korea
Phone: 82 (2) 753-7911 Fax: 82 (2) 756-4972

HORIBA Instruments (Singapore) Pte Ltd. Singapore

3 Changi Business Park Vista #01-01 Akzonobel House, Singapore 486051
Phone: 65 (6) 745-8300 Fax: 65 (6) 745-8155

HORIBA Vietnam Co., Ltd. Vietnam

Unit 6, 10 Floor, CMC Tower, Duy Tan Street, Dich Vong Hau Ward, Cau Giay District, Hanoi, Vietnam
Phone: 84 (4) 3795-8552 Fax: 84 (4) 3795-8553

HORIBA (Thailand) Ltd. Thailand

East Office
850 / 7 Soi Lat Krabang 30 / 5, Lat Krabang Road, Lat Krabang, Bangkok 10520, Thailand
Phone: 66 (0) 2734 4434 Fax: 66 (0) 2734 4438

PT HORIBA Indonesia Indonesia

Jl. Jalur Sutera Blok 20A, No.16-17, Kel. Kunciran, Kec. Pinang Tangerang-15144, Indonesia
Phone: 62 (21) 3044-8525 Fax: 62 (21) 3044-8521

HORIBA India Private Limited India

Delhi
246, Okhla Industrial Estate, Phase 3 New Delhi-110020, India
Phone: 91 (11) 4646-5000 Fax: 91 (11) 4646-5020
Technical Center
D-255, Chakan MIDC Phase-II, Bhamboli Village, Pune-410501, India
Phone: 91 (21) 3567-6000
Bangalore
No.55, 12th Main, Behind BDA Complex, 6th sector, HSR Layout, Bangalore South, Bangalore-560102, India
Phone: 91 (80) 4127-3637

HORIBA Instruments Inc. USA

Head Office
9755 Research Drive, Irvine, CA 92618, U.S.A.
Phone: 1 (949) 250-4811 Fax: 1 (949) 250-0924
Houston
5390 Bay Oaks Drive, Pasadena, TX 77505, USA
Phone: 1 (281) 482-4334 Fax: 1 (281) 614-0303

HORIBA Instruments Brazil, Ltda. Brazil

Head Office
Rua: Presbitero Plinio Alves de Souza, 645, Loteamento Polo Multivas Barirro Medeiros-Jundiai Sao Paulo CEP 13.212-181 Brazil
Phone: 55 (11) 2923-5400 Fax: 55 (11) 2923-5490

HORIBA France SAS France

Les Ulis
12, Av des Tropiques Hightec Sud, F-91955 Les Ulis, France
Phone: 33 (1) 69-29-96-23 Fax: 33 (1) 69-29-95-77

HORIBA UK Limited UK

Northampton
Kyoto Close Moulton Park, Northampton NN3 6FL, UK
Phone: 44 (1604) 542-5000 Fax: 44 (1604) 542-699

HORIBA Europe GmbH Germany

Head Office
Hans-Mess-Str. 6 D-61440 Oberursel Germany
Phone: 49 (6172) 1396-0 Fax: 49 (6172) 1373-85
Leichlingen
Julius-kronenberg Str.9 D-42799 Leichlingen Germany
Phone: 49 (2175) 8978-0 Fax: 49 (2175) 8978-50

HORIBA Czech Czech

Prumyslova 1306 / 7, CZ-10200, Praha 10, Czech Republic
Phone: 420 (2) 460-392-65

HORIBA (Austria) GmbH Austria

Kaplanstrasse 5 A-3430 Tulln, Austria
Phone: 43 (2272) 65225 Fax: 43 (2272) 65230